


C3000 Series

- [Specifications C3010 and C3030](#)

Mind that the model C3010 has been upgraded since September 2014 with Dissolved Oxygen measurements. The model C3020 became obsolete.

- [Specifications C3040](#)
- [Specifications C3050](#)
- [Specifications C3060](#)

Info

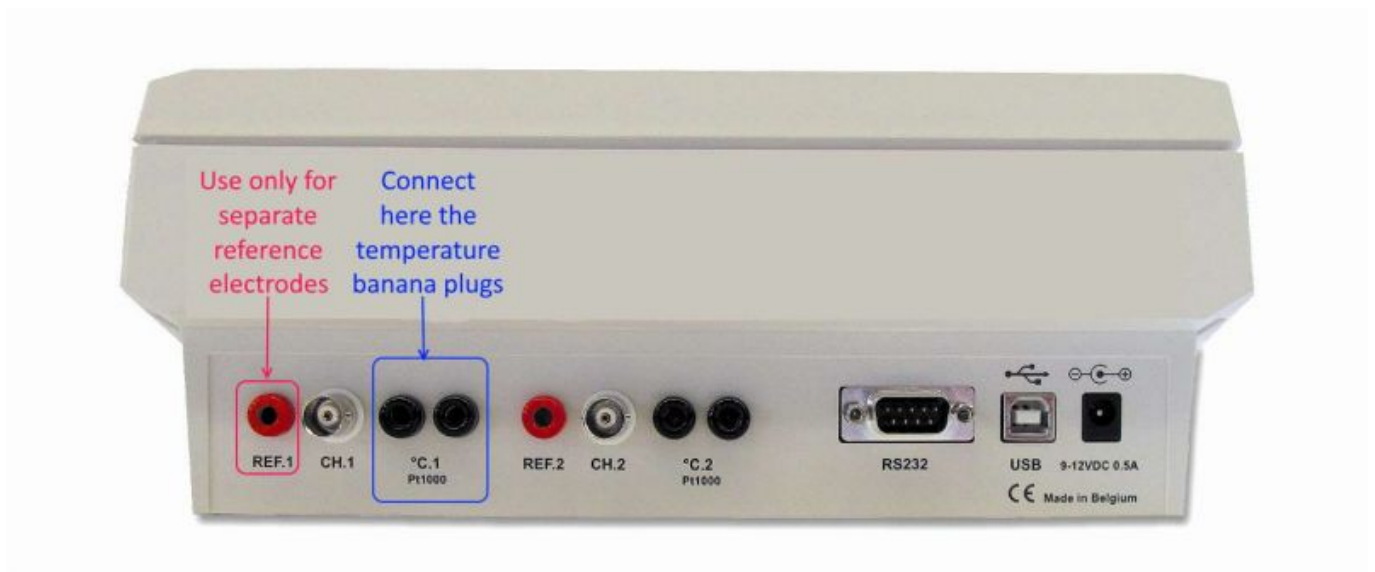

- [C30xx Manual](#)

Info

- [IQ/OQ/PQ documents](#)

Software

- [Firmware of the devices](#)
- [Software DIS1](#)
- [Digital communication commands](#)

From:

<http://www.consort.be/wiki/> - **Support website**

Permanent link:

<http://www.consort.be/wiki/c30xx>

Last update: **26/09/2018 12:10**

